





Thigh System

User's Reference Card


L360™
Thigh System







Putting On the L360 Thigh Cuff

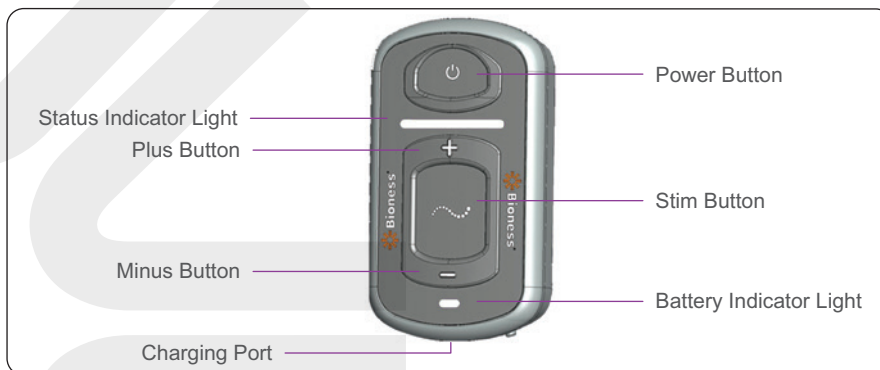- 1 Wet and attach the Thigh Cloth Electrodes to the L360 Thigh Cuff.
- 2 For placement on the quadriceps while seated, place the L360 Thigh Cuff on your thigh, positioning at the midline of the thigh and center on bulk of quadriceps muscle.
- 3 Make sure to place the L360 Thigh Cuff in the fitting position determined by your clinician. See Figure 3 (Front view – Quadriceps).
- 4 For placement on hamstrings, while seated or standing, place the L360 Thigh Cuff at the midline of the thigh and center on bulk of hamstring muscle, right under the gluteal fold. See Figure 4 (Back view – Hamstrings).



Operating the L360 Thigh System



- 1 Press the  on/off button to turn on the EPG.
- 2 Select either gait or training mode:
 - To select gait mode, press the  mode button *briefly*.
 - To select training mode, press and *hold* the  mode button for 3 seconds. The EPG will acknowledge the new mode with audio and tactile feedback. To exit training mode, press and hold the  mode button for 3 seconds.
- 3 If necessary, adjust the stimulation intensity level by pressing the  plus or  minus button.

For a complete list of all contraindications, warnings, adverse reactions, precautions, and care instructions please review the User's Guide.

Bioventus and the Bioventus logo are registered trademarks of Bioventus LLC.
L360, Bioness and the Bioness Logo are trademarks of Bioness Inc. in the United States or other countries | BionessRehab.com
© 2022 Bioventus LLC 612-01411-001 Rev. A 12/2022





 **bioness**[®]
A Bioventus Rehab Company

Rx Only (US only)

Charging the Batteries






Connect the system charger set to the EPG, then plug into a wall socket.



 (flashing)	EPG Status Indicator Bar Flashes Red along with Battery Indicator Light Flashing Yellow	EPG Low Battery
 (flashing)	Flashes Yellow	Low Battery
 (flashing)	Flashes Green	Charging
 (flashing)	Solid Green	Fully Charged








EPG Displays



 (flashing)	Flashes Green	System is On
	Flashes Green	Stimulation is Off
 (flashing)	Flashes Yellow	Stimulation is On
 (flashing)	Flashes Red with Audible Alarm	Active Error
	Solid Red	EPG Malfunction

Control Unit Displays (Optional)



	Solid	System is On
	Stim Wave Visible	System is in Gait/Training, Stimulation is enabled but Off
	Stim Wave Flashes	System is in Gait/Training, Stimulation is enabled and On
	Displays 0–9	Intensity Level
	Displays Gait Icon	Gait Mode is Enabled
	Displays Training Icon	Training Mode is Enabled
	Displays Audio Icon	Audio is On

